



King's Research Portal

DOI:

[10.5281/zenodo.495887](https://doi.org/10.5281/zenodo.495887)

Document Version

Publisher's PDF, also known as Version of record

[Link to publication record in King's Research Portal](#)

Citation for published version (APA):

Charlton, P. H., Camporota, L., Smith, J., Chaffey, G., Nandi, M., Christie, M. I., Aston, P., Beale, R., & Alastruey-Armon, J. (2017). Clinical Applications of Attractor Reconstruction Analysis. <https://doi.org/10.5281/zenodo.495887>

Citing this paper

Please note that where the full-text provided on King's Research Portal is the Author Accepted Manuscript or Post-Print version this may differ from the final Published version. If citing, it is advised that you check and use the publisher's definitive version for pagination, volume/issue, and date of publication details. And where the final published version is provided on the Research Portal, if citing you are again advised to check the publisher's website for any subsequent corrections.

General rights

Copyright and moral rights for the publications made accessible in the Research Portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognize and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the Research Portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the Research Portal

Take down policy

If you believe that this document breaches copyright please contact librarypure@kcl.ac.uk providing details, and we will remove access to the work immediately and investigate your claim.

Clinical Applications of Attractor Reconstruction Analysis



P.H. Charlton^{1,2}, L. Camporota², J. Smith², G. Chaffey³,
M. Nandi¹, M. Christie¹, P.J. Aston³, R. Beale², J. Alastruey¹

¹ King's College London

² Guy's and St Thomas' NHS Foundation Trust

³ University of Surrey




1. Analysing pulse waveforms using Attractor Reconstruction (AR)

Pulse waveforms contain a wealth of information


Blood pressure and pulse oximetry signals are routinely acquired during physiological assessments. These pulse waveforms contain much physiological information (see right). Currently only simple measures such as heart rate and blood pressure values are routinely extracted from them.

Physiological information in a pulse waveform

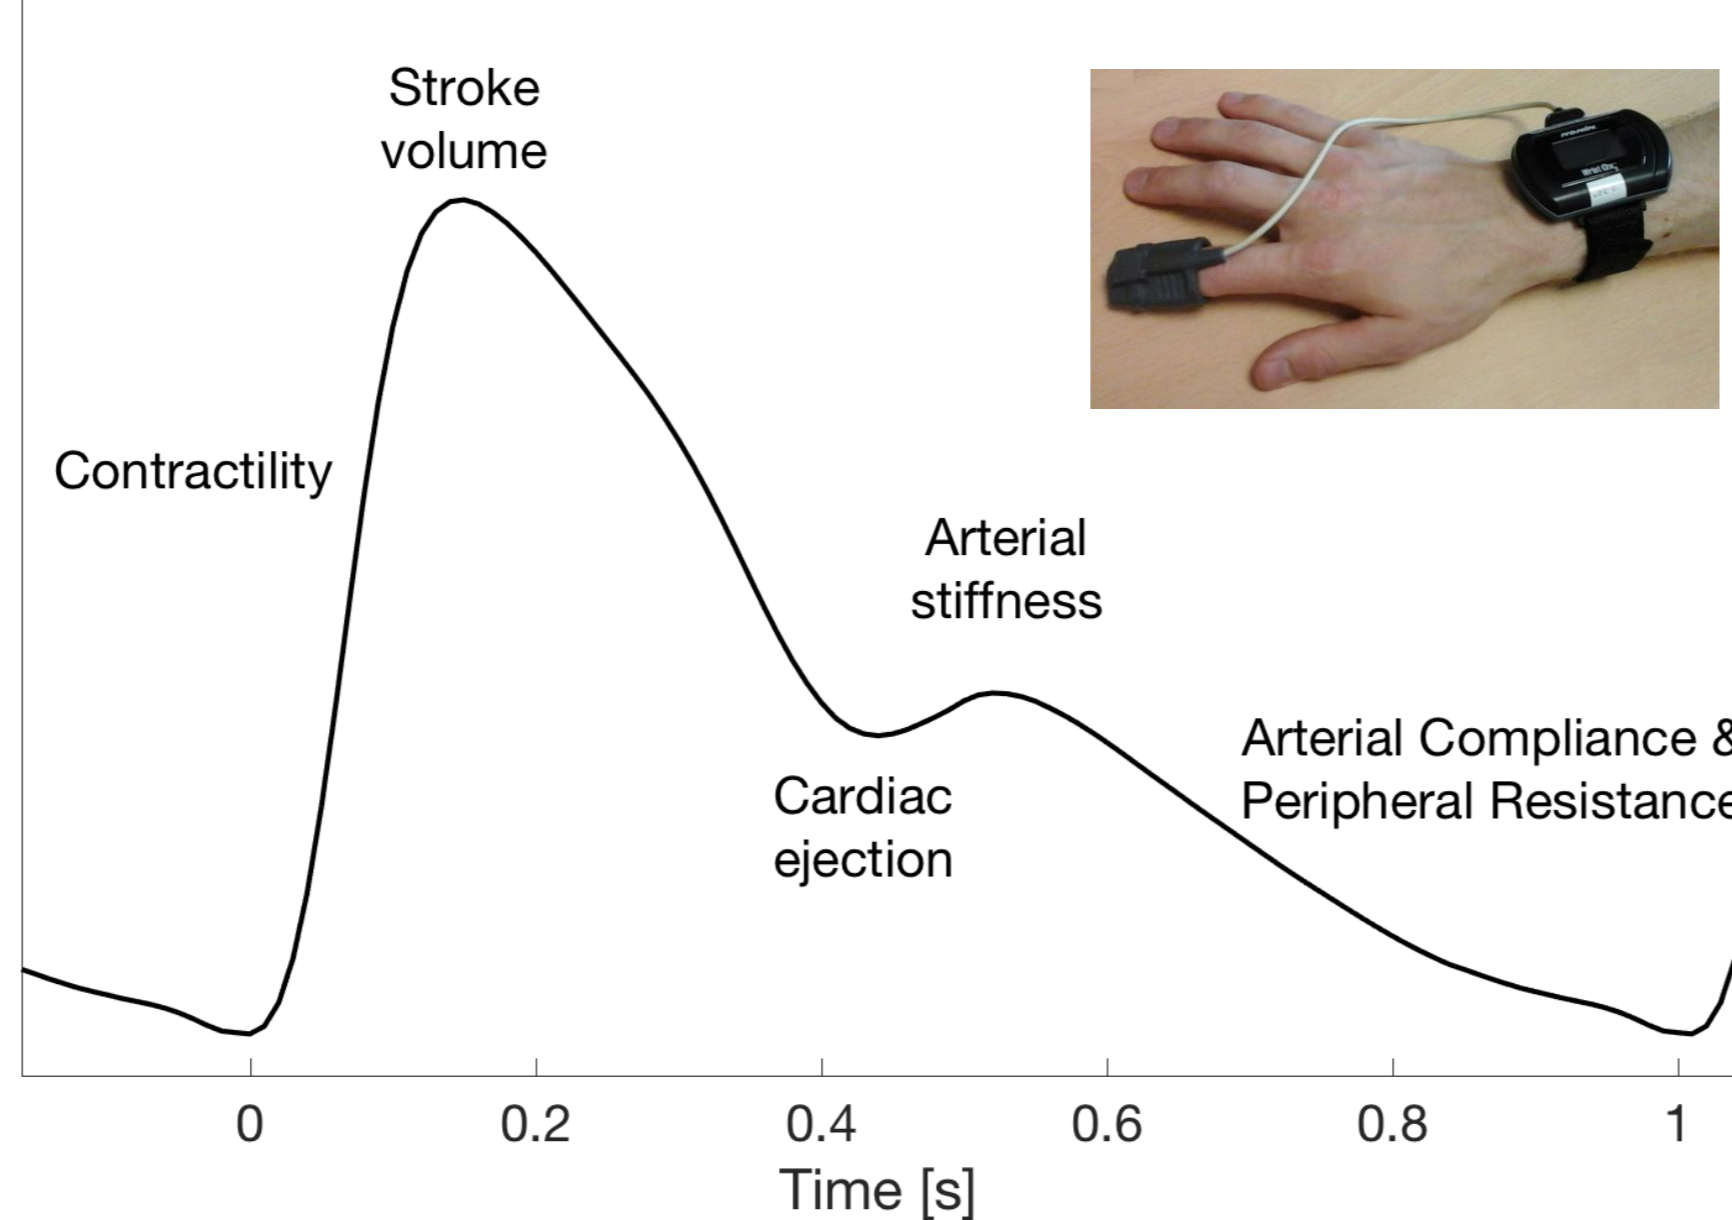

Attractor Reconstruction (AR)

AR is a novel mathematical technique for analysing periodic signals. It transforms a **signal** into an **attractor** (see right). The resulting attractor can be used to extract information on the variability and shape of the signal. Changes in the shape or variability of an attractor may indicate changes in cardiovascular health, or disease progression.

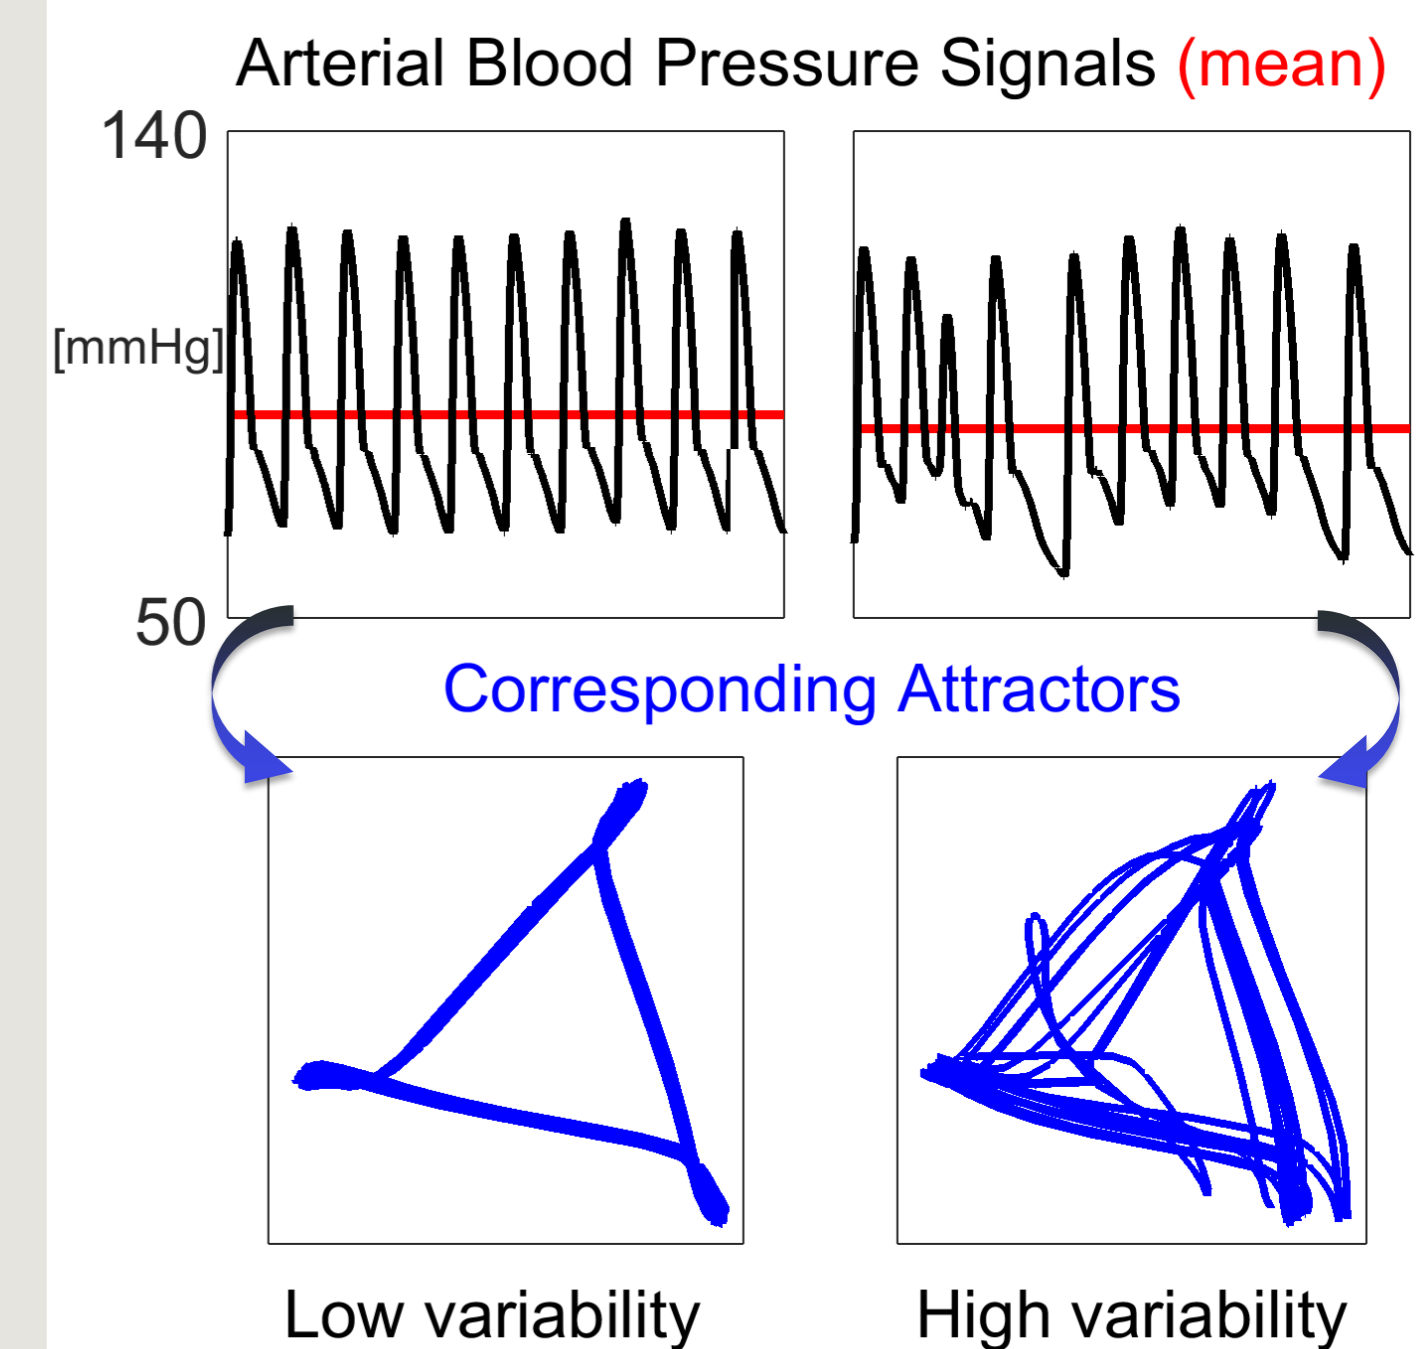


2. Physiological Insights

Vascular Properties

The properties of the smaller arteries affect the morphology of attractors obtained from a pulse oximetry waveform. This is demonstrated for vascular stiffness and diameter below.

Increasing vascular stiffness

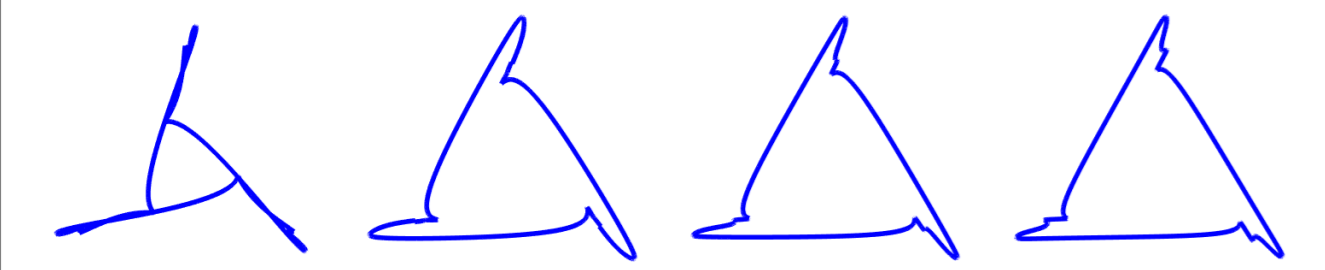


Increasing vascular diameter




Cardiac Properties

The properties of the heart affect attractors, even when measured distally using a pulse oximeter waveform. Two examples are shown below: ejection time and heart rate.

Increasing ejection time

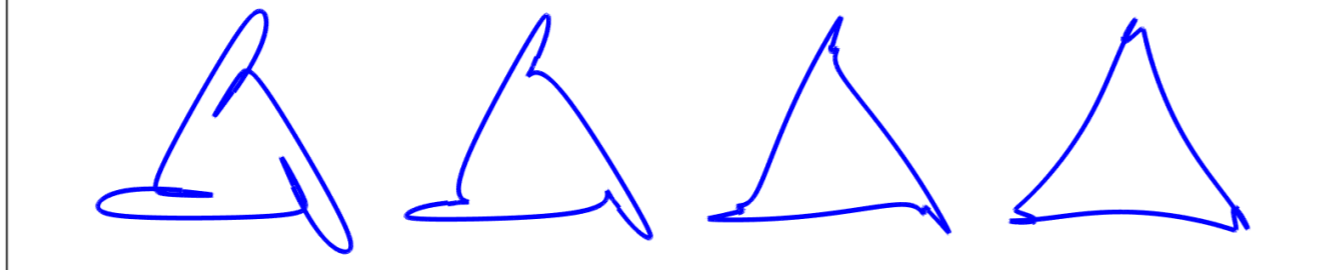


Increasing heart rate

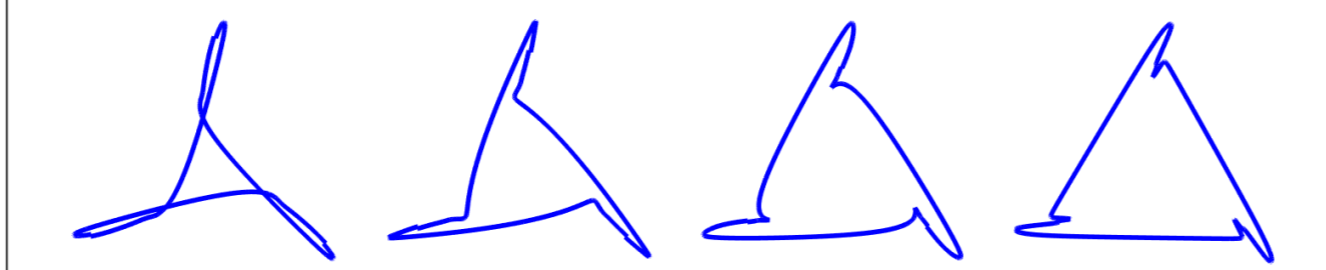


Physiological State

The changes shown to the left were obtained from simulations of blood flow. Changes in attractors are also observed during physiological changes, as shown below.

Increasing age

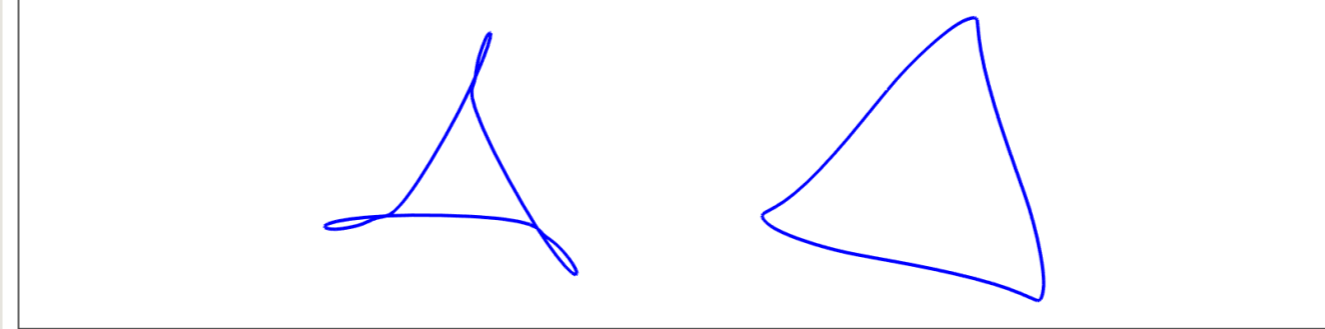


Recovery from exercise

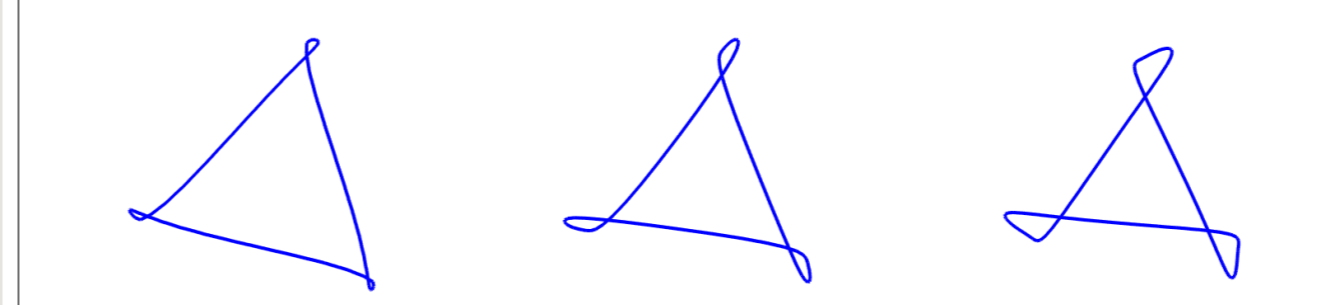


Measurement Site

The morphology of attractors varies according to the site at which they are measured, as shown by the four blood pressure attractors below.

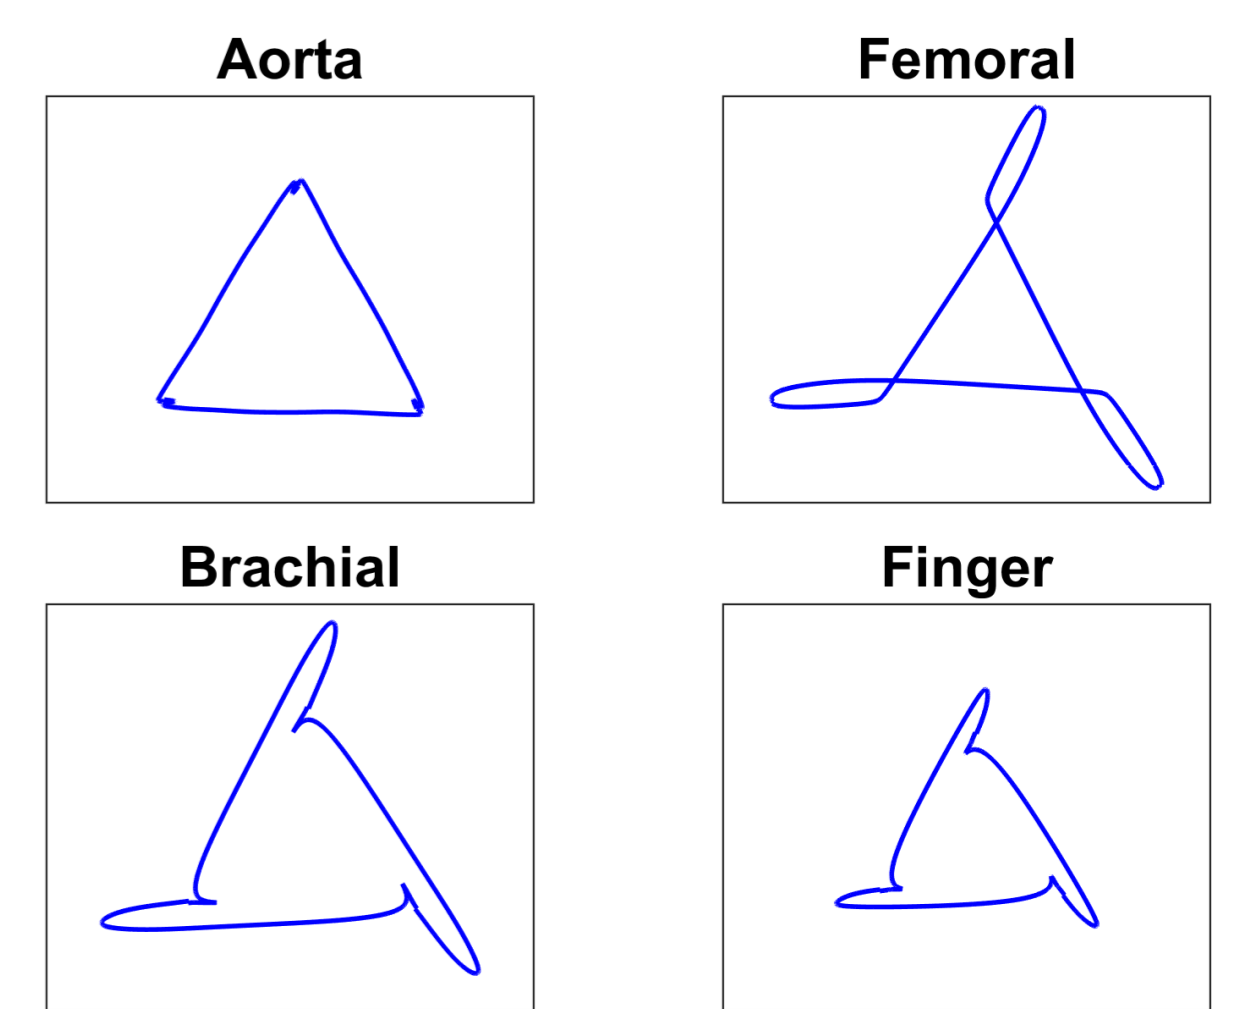

3. Detection of Sepsis

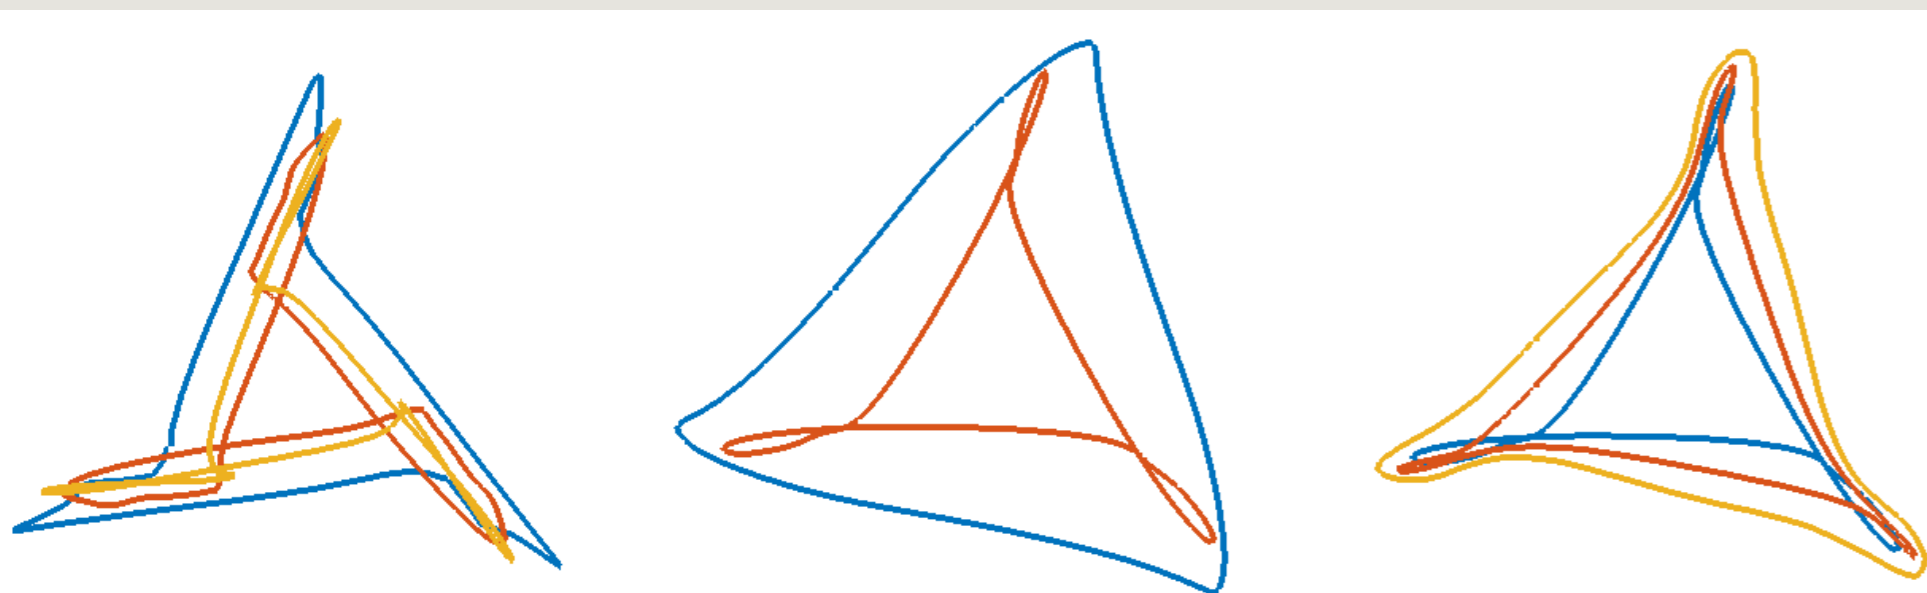


Changes in attractor shape which may be associated with the progression of sepsis

AR may provide early detection of sepsis

Sepsis is a heightened response to infection, which increases morbidity and mortality. Early detection is essential to prevent its progression. AR may allow markers of sepsis to be derived from physiological signals. This is due to the impact of sepsis on the cardiac, vascular and autonomic nervous systems, all of which influence the pulse waveform.


4. Respiratory Monitoring

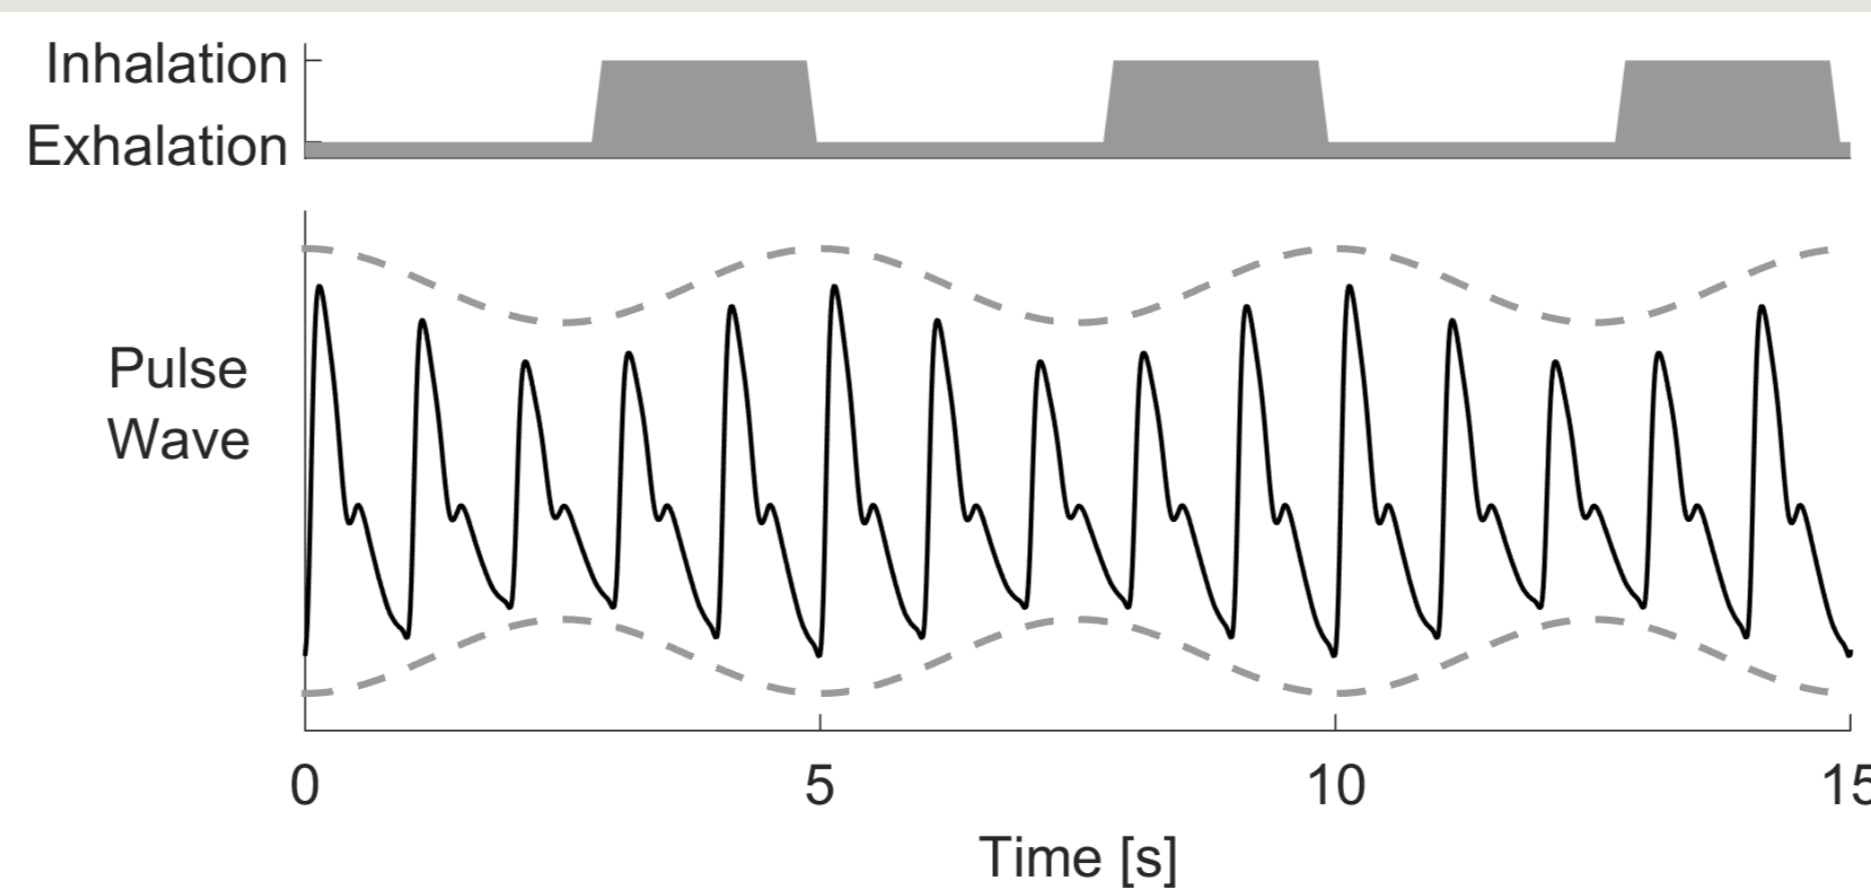

AR can improve respiratory rate (RR) estimation from the pulse oximeter

RR is usually measured by manually counting breaths. Techniques have been developed to estimate RR electronically from the pulse oximetry signal, although these are susceptible to inaccuracies. We have used AR to improve the accuracy of RRs derived from a pulse oximeter.

5. Measurement Accuracy

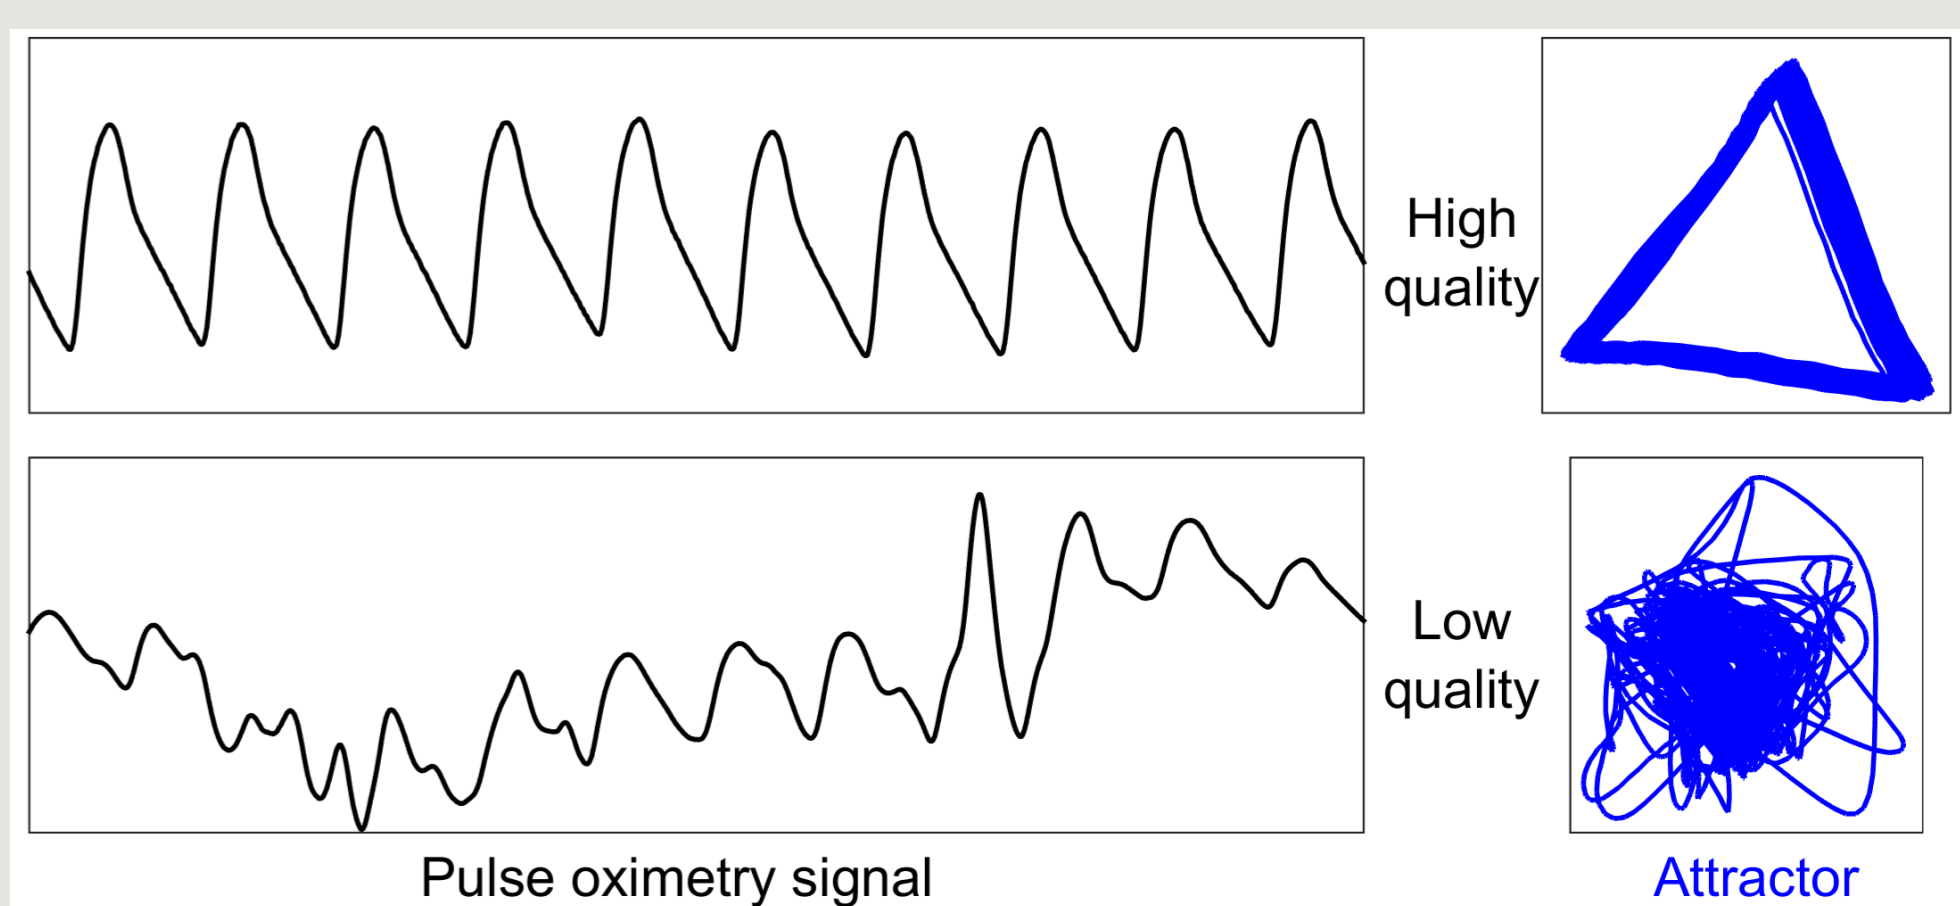

AR can be used to identify and eliminate inaccurate clinical measurements

Several clinical measurements are derived from physiological signals. The signals must be of high quality to ensure accurate measurements. Attractors change dramatically during periods of low signal quality. Therefore, AR could be used to automatically discard inaccurate measurements.